

# Assessment of spatiotemporal gait parameters using a deep learning algorithm-based markerless motion capture system

Robert Kanko<sup>1\*</sup>, Gerda Strutzenberger<sup>2</sup>, Marcus Brown<sup>3</sup>, Scott Selbie<sup>3</sup>, Kevin Deluzio<sup>1</sup>

<sup>1</sup>Department of Mechanical & Materials Engineering, Queen's University, Kingston, Canada

<sup>2</sup>Department of Sport and Exercise Science, University of Salzburg, Salzburg, Austria

<sup>3</sup>Theia Markerless Inc., Kingston, Canada

\*Correspondence: r.kanko@queensu.ca

## Abstract

**Background:** Spatiotemporal parameters can characterize the gait patterns of individuals, allowing assessment of their health status and detection of clinically meaningful changes in their gait. Video-based markerless motion capture is a user-friendly, inexpensive, and widely applicable technology that could reduce the barriers to measuring spatiotemporal gait parameters in clinical and more diverse settings.

**Research Question:** Do spatiotemporal gait parameters measured using *Theia3D* markerless motion capture demonstrate concurrent validity with those measured using marker-based motion capture?

**Methods:** 30 healthy adult participants performed treadmill walking at self-selected speeds while 2D video and marker-based motion capture data were collected simultaneously. Kinematic-based gait events were used to measure nine spatiotemporal gait parameters from both systems independently. The parameters were compared using their group means, Bland-Altman methods, Pearson correlation coefficients, paired-samples *t*-tests, and intraclass correlation coefficients ( $ICC_{(A-1)}$  and  $ICC_{(C-1)}$ ).

**Results:** Group means between marker-based and markerless methods were indistinguishable across all nine gait parameters, and the Bland-Altman plots showed no systematic biases or clinically meaningful differences between the systems. Pearson correlation coefficients indicated perfect or near-perfect correlation ( $r \geq 0.96$ ) between systems for gait speed, cadence, step time, step length, stride length, stride width and stance time, and strong correlations ( $r \geq 0.87$ ) for double-limb support time and swing time. *T*-tests indicated differences in stance, swing, and double-limb support time parameters. Strong correlations were found for both ICCs, with the lowest being  $ICC_{(A-1)}$  of 0.84 for both double-limb support time and swing time.

**Significance:** The high level of agreement and correlation between both systems indicate that the *Theia3D* markerless motion capture system is sufficiently accurate for measuring spatiotemporal gait parameters for research, clinical, and other uses. The results presented here for healthy adults during treadmill walking do not necessarily reflect the performance of the markerless system under different conditions.

**Keywords:** markerless motion capture; spatiotemporal parameters; gait analysis; deep learning.

## 1. Introduction

Gait analysis is a useful tool for assessing and comparing human movement patterns to gain insight into a variety of health-related factors. Marker-based optoelectronic motion capture has often been considered the ‘gold standard’ for gait analysis, but its high cost and requirements for experienced operators and dedicated laboratory space have prompted the development and validation of alternative technologies. Some examples of alternative technologies include instrumented walkways [1], depth sensors [2], photoelectric cell systems [3], inertial measurement units [4], and in-shoe pressure sensors [5]. However, these technologies still require expensive equipment, and may have limited options for deployment or provide minimal data. Two-dimensional (2D) video-based markerless motion capture is an emerging technology that has the potential to accurately measure human motion and eliminate issues associated with marker-based motion capture and other alternative technologies. Several different approaches to 2D video-based markerless motion capture have been developed and implemented to varying levels of success, feature recognition being one such approach [6–8]. Feature recognition employs deep learning techniques such as neural networks to identify and track the movement of specific anatomical landmarks in single or successive photographic images. This process allows the pose of human subjects to be estimated based on the positions of the tracked anatomical landmarks. The feature recognition approach to 2D video-based markerless motion capture has several benefits over depth sensor-based approaches such as the Microsoft Kinect or video-based surface registration approaches, two alternative approaches to markerless motion capture. Some benefits include there being no need for specific technology, no need to separate or subtract the background of the image from the subject, and the ability to make pose estimates despite occlusion of the subject. Feature recognition has been implemented in *Theia3D* software (Theia Markerless Inc., Kingston, ON) using an array of synchronized and calibrated 2D video cameras and a deep convolutional neural network to estimate human pose in three-dimensions (3D). *Theia3D* has the potential to precisely determine the pose of humans during any dynamic activity, wearing any clothing, and in any environment, which would drastically increase the ease of and opportunities for collecting human movement data. If this technology is capable of measuring spatiotemporal gait parameters with similar accuracy to marker-based motion capture, it would increase the opportunities to apply the findings of clinical gait research and their impact on patient outcomes. These spatiotemporal gait parameters have been shown to be useful clinical measures that can detect ‘negative’ changes in individuals’ gait patterns due to pathology [9–12] or aging [13], and ‘positive’ changes due to rehabilitation [14,15] or locomotor training [16–18]. However, it is crucial that they are obtained using objective techniques to ensure adequate accuracy and repeatability [19].

The objective of this work was to determine if the spatiotemporal gait parameter measurements obtained by using the *Theia3D* markerless motion capture system were equivalent to those from a field-accepted marker-based motion capture system during treadmill walking gait.

## 2. Methods

### 2.1 *Theia3D* Markerless Motion Capture

*Theia3D* is a markerless motion capture software that performs 3D pose estimation using artificial intelligence, specifically deep learning. Cameras are placed to establish a 3D volume captured by their 2D views and calibrated to determine their position and orientation in 3D space. For this work, calibration was performed using a marked wand with known dimensions since the cameras used could be calibrated in this way; however, the use of other calibration objects with known dimensions is

supported by the software. The calibrated cameras synchronously record video data while the subject performs a task in the capture volume. Given these synchronized video data, *Theia3D* performs feature extraction on the 2D images to identify and locate anatomical landmarks and joint positions in 3D space. This feature detection is performed using deep convolutional neural networks that are trained on a dataset of over 500,000 images, which included images from a proprietary dataset and Microsoft COCO [20]. These images, which show humans in a wide array of settings, clothing, and performing various activities, had their anatomical landmarks and joint positions manually labelled by highly trained annotators. Quality assurance was performed on all labelled points by a second individual. The visual features that correspond to these keypoints were learned by the algorithm, and once learned can be applied to any image. Given an input image and the known camera locations, the algorithm detects and locates the keypoints in 3D, then applies an articulated multi-body model from which the motion of the subject is measured.

## 2.2 Participants

Thirty healthy, recreationally active individuals (15 male/15 female, mean (SD) age: 23.0 (3.5) years, height: 1.76 (0.09) m, weight: 69.2 (11.4) kg) were recruited to participate in this study at the Human Mobility Research Laboratory in Kingston, Ontario. Participants gave written informed consent and this study was approved by the institutional ethics committee. Exclusion criteria included having suffered any lower-limb injuries in the previous 9 months, having any neuromuscular, musculoskeletal or metabolic impairments that could prevent their performance of walking, running, or jumping tasks, or currently taking medication for any neurological, cardiovascular, or metabolic disorders.

## 2.3 Experimental Setup

Participants walked on a treadmill while two camera systems were used to simultaneously capture their movement: a marker-based camera system consisting of seven Qualisys 3+ cameras (Qualisys AB, Gothenburg, Sweden) which recorded marker trajectories, and a markerless camera system consisting of eight Qualisys Miquis cameras (Qualisys AB, Gothenburg, Sweden) which recorded 2D video. These cameras were used for the purpose of this comparison since their data could be spatially and temporally synchronized by connecting them to a single instance of Qualisys Track Manager (Qualisys AB, Gothenburg, Sweden). However, any system consisting of at least two synchronized video cameras would be sufficient to collect similar data. Both systems collected data at 85 Hz and were calibrated simultaneously using a marked wand of known dimensions, resulting in one shared global reference frame. These factors permitted a fair comparison of the two systems.

## 2.4 Experimental Procedure

Participants wore minimal, tightly fitting clothing typical of marker-based motion capture methods, and their personal running shoes. Retroreflective markers were affixed to relevant anatomical landmarks and rigid clusters of retroreflective markers were affixed to the shanks and thighs. Starting at an initial speed of 1.2 m/s, participants walked on the treadmill and determined a comfortable, self-selected walking speed. Following an acclimatization period of two minutes, ten consecutive four-second trials were collected.

## 2.5 Data Analysis

Marker-based motion capture data were tracked in Qualisys Track Manager and the 2D video data for markerless motion capture were processed in *Theia3D* to obtain 3D pose estimates of each body segment. The tracked marker data and the markerless 3D pose estimates, which were exported as 4x4 pose matrices, were both analyzed further using Visual3D.

In Visual3D, two skeletal models (one for marker-based and one for markerless) with homologous segments were defined from a static posture such that their segment local coordinate systems were identical in this static posture. These two models used independent tracking data; one tracked the 3D marker trajectories (marker-based), while the other tracked the 4x4 pose matrices (markerless). These models were generated for every participant and applied to all trials collected from the respective participant.

Independent, kinematically-defined gait events were generated for the marker-based and markerless models using the method described by Zeni Jr. *et. al.* [21]. This method detects heel-strike and toe-off events using kinematic data of the metatarsal head and heel markers. In order to determine these events using the markerless motion capture system, virtual markers were added to the markerless model at the same positions as those real markers in the static posture, but which tracked the motion of the markerless model's feet. If this method were to be used without the presence of markers, the anatomical landmarks identified by the markerless system could be used to generate the virtual markers instead. The independent gait events were used to measure the time- and distance-based spatiotemporal gait parameters of each participant from both motion capture systems separately. The gait parameters were measured for all strides within the ten four-second trials and a mean of both sides of the body was obtained for each subject. The parameters compared in this work were gait speed, cadence, step time, stance time, swing time, double-limb support time, step length, stride length, and stride width, and are described in further detail in Table 1. Parameters were computed in Visual3D and exported to MATLAB (MathWorks, Natick, MA) for further analysis.

**Table 1:** Descriptions of the included spatiotemporal gait parameters.

Gait Parameter	Description
Gait Speed	Distance covered per second, calculated as the measured stride length divided by the measured stride time, reported in meters per second [m/s].
Cadence	Rate of leg turnover, calculated as 60 seconds divided by the measured step time, reported in steps per minute [steps/min].
Step Time	Time elapsed between heel-strike of the contralateral foot and the successive heel-strike of the ipsilateral foot, reported in seconds [s].
Stance Time	Time elapsed between heel-strike of the ipsilateral foot and the successive toe-off of the same foot, reported in seconds [s].
Swing Time	Time elapsed between toe-off of the ipsilateral foot and the successive heel-strike of the same foot, reported in seconds [s].
Double-Limb Support Time	Time elapsed while both feet are in contact with the ground and taken as the sum of the two instances of double-limb support during one gait cycle, reported in seconds [s].


Step Length	Distance from the position of the proximal contralateral foot (ankle joint) at the previous contralateral heel-strike to the position of the proximal ipsilateral foot (ankle joint) at the ipsilateral heel-strike taken in the direction of progression, reported in centimeters [cm].
Stride Length	Distance from the position of the proximal ipsilateral foot (ankle joint) at ipsilateral heel-strike to the position of the proximal ipsilateral foot (ankle joint) at the successive ipsilateral heel-strike taken in the direction of progression, reported in centimeters [cm].
Stride Width	Perpendicular distance between the position of the proximal contralateral foot (ankle joint) at contralateral heel-strike to the vector between positions of the proximal ipsilateral foot (ankle joint) at successive ipsilateral heel-strikes, reported in centimeters [cm].

### 2.6 Statistical Analysis

Means and standard deviations for each gait parameter were calculated for each subject and across all subjects. Bland-Altman methods were used to compare the measurements taken by both systems on each subject by plotting the difference between the two measurements made on each subject against the average of the two measurements, providing insight into the bias and variability in the differences between the systems [22]. Limits of agreement (LoA) were included to show the range of differences between measurements that could be expected from the two systems, and 95% confidence intervals were used to show the possible range over which the LoA could have been found (Carkeet, 2015). Pearson's correlation coefficient ( $r$ ) was calculated to assess the correlation between the markerless and marker-based systems and paired-samples  $t$ -tests were used to detect significant differences between the sample means. Intraclass correlation coefficients (ICC) of the form (C-1) and (A-1) were calculated to assess consistency between measurement systems and agreement within subjects, respectively [23].


### 3. Results


The independent kinematic gait events determined from the marker-based and markerless models were found to have high agreement across all subjects, with greater than 80% of all events detected within two frames of each other (time difference  $<0.0235$  seconds) and only 3% of events detected more than four frames apart (0.0471 seconds). The distributions of the differences between the gait events obtained from the marker-based and markerless models are shown in Figure 1.

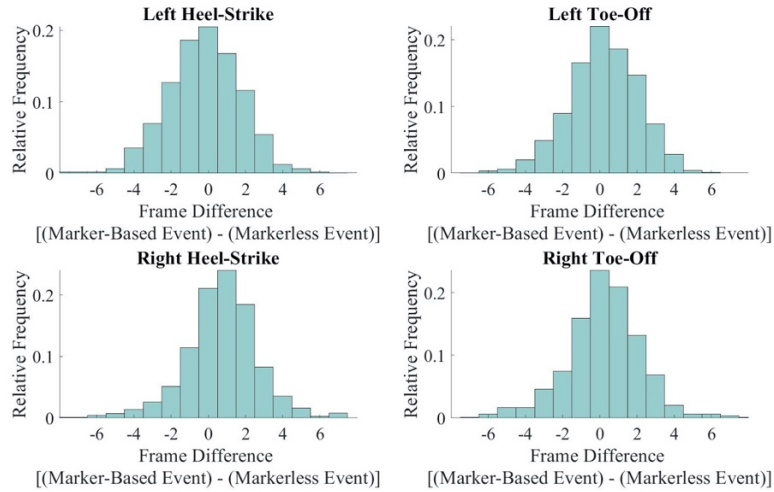

**Figure 1:** Relative frequency distributions of the difference between independent kinematic gait events detected based on the marker-based and markerless models, where the difference is calculated as (marker-based event frame number) - (markerless event frame number).

Means and standard deviations across all 30 subjects for the nine spatiotemporal gait parameters included were found to be nearly identical when measured by the marker-based and markerless motion capture systems (Table 2, Figure 2, Supplementary Material). Mean gait speed was 1.41 m/s for both the marker-based and markerless systems, compared to 1.40 m/s calculated using the actual treadmill belt speed. The sample means measured by both systems were identical for cadence, step time, stance time, swing time, stride length, and stride width, and varied minimally for mean double-limb support time and step length. Violin and Bland-Altman plots for gait speed, cadence, and step length are included as examples in Figure 2; the remaining gait parameter figures are included in the Supplementary Material.

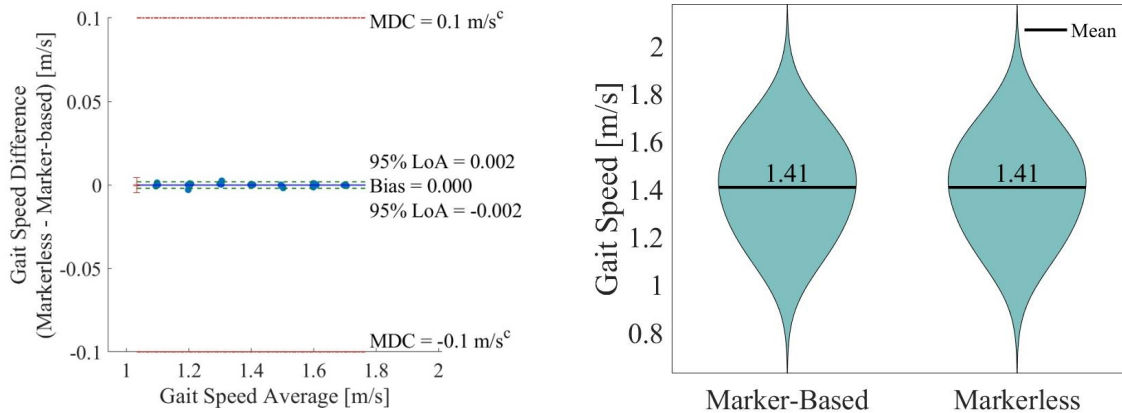

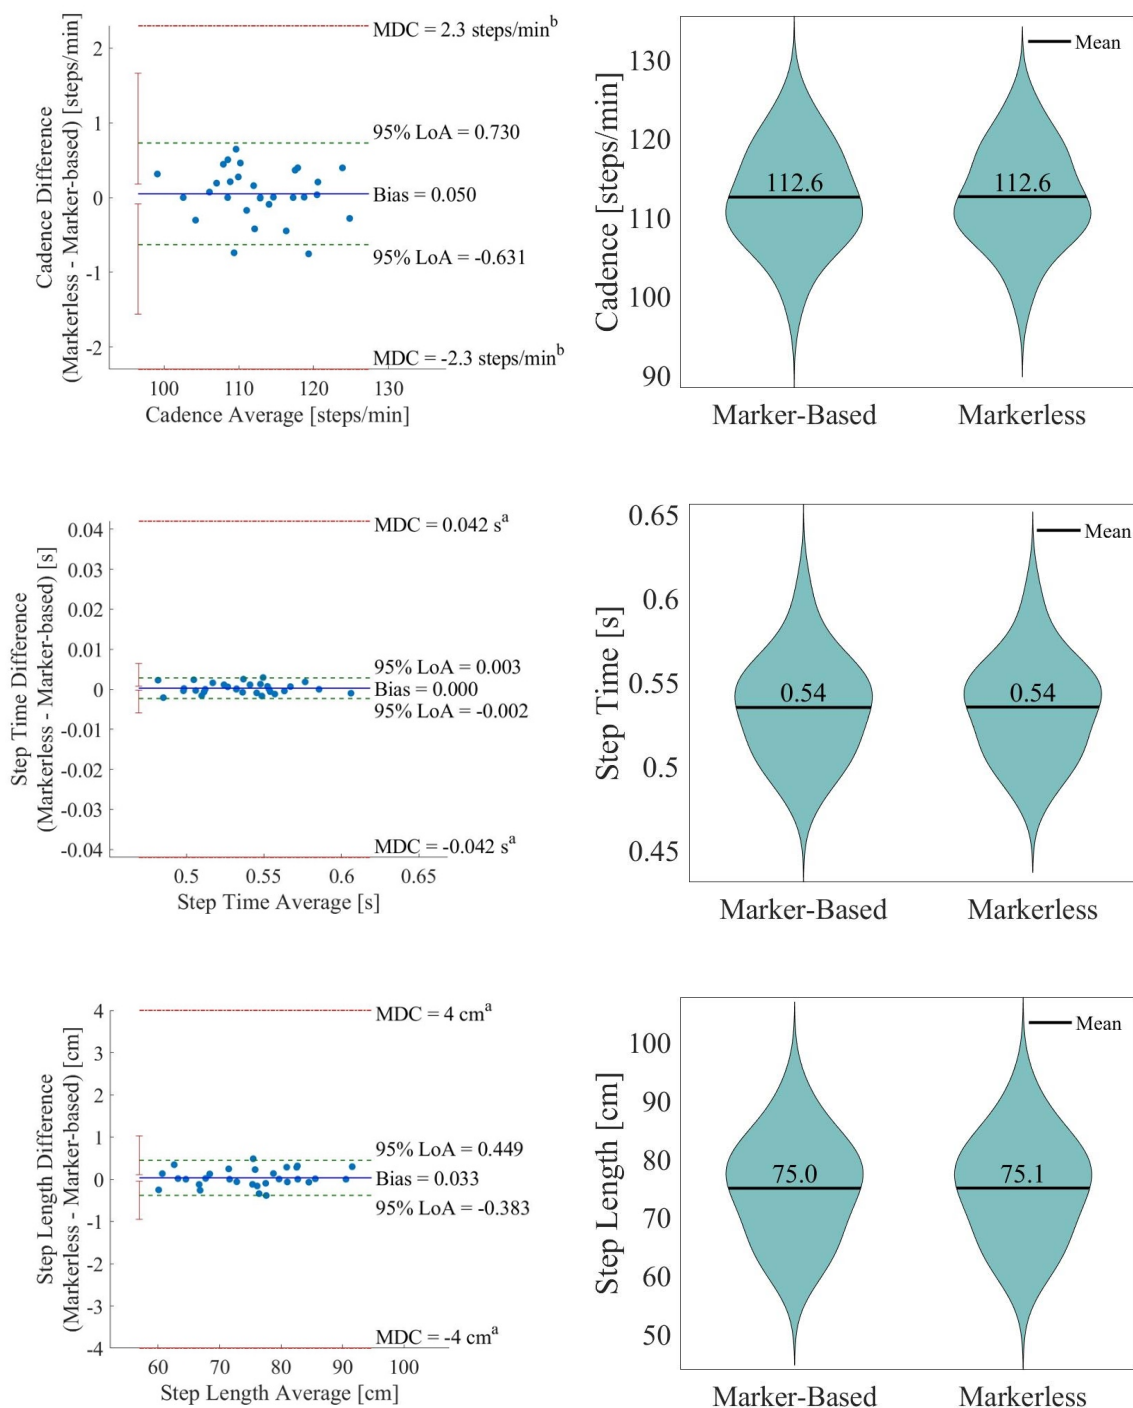

**Figure 2:** Bland-Altman and violin plots of gait speed, cadence, step time, and step length measurements. Bland-Altman plots show the difference between the marker-based and markerless measurements against the average of the marker-based and markerless measurements. Violin plots show the distribution of the marker-based and markerless measurements for all thirty subjects. Minimal detectable change values used are from <sup>a</sup>[33], <sup>b</sup>[34], <sup>c</sup>[35].

Differences in the gait parameters measured by the marker-based and markerless motion capture systems were very small and randomly distributed for all parameters as demonstrated by the Bland-

Altman plots (Figure 2, Supplementary Materials). No relationships between the level of difference and the average measurement were visually observed, indicating there is no proportionality bias between the two systems. The biases between system measurements were very small for all gait parameters, with several parameters demonstrating no bias. The 95% limits of agreement were generally distributed equally on either side of the bias. The 95% confidence intervals on the limits of agreement were within the minimal detectable change (MDC) values from the literature in all cases except stance time and swing time. The positive and negative stance time confidence intervals and the positive swing time confidence interval extended slightly beyond the minimal detectable change, indicating there is a possibility that those limits of agreement could have been found slightly outside of the MDC range.

The sample distributions from the marker-based and markerless motion capture systems shown in the violin plots were nearly indistinguishable for all included parameters (Figure 2, Supplementary Materials). The Pearson correlation coefficients indicated perfect correlation between the marker-based and markerless motion capture systems' measurements of gait speed, cadence, step time, step length, and stride length (Table 2). Stance time and stride length also demonstrated very high correlation between systems, while swing time and double-limb support time had the lowest correlation coefficients of 0.88 and 0.87, still indicating excellent agreement ( $ICC > 0.75$ , Cicchetti, 1995) between the markerless and marker-based systems for all gait parameters (Table 2). No significant differences between the marker-based and markerless measurements of gait speed, cadence, step time, step length, stride length, and stride width were found based on paired-samples *t*-tests (Table 2).

**Table 2:** Comparison of spatiotemporal gait parameter measurements obtained from the marker-based and markerless motion capture systems, including means, standard deviations, Bland-Altman biases and limits of agreement, paired samples *t*-test *p*-values, Pearson's correlation coefficients (*r*), and intraclass correlation coefficients (ICCs) for consistency and agreement between measurement systems.

Gait Parameter	Marker-Based Mean (SD)	Markerless Mean (SD)	B-A Bias (95% LoA)	<i>P</i> -value	<i>r</i>	Consistency ICC (C-1)	Agreement ICC (A-1)
Gait Speed [m/s]	1.41 (0.19)	1.41 (0.19)	0.00 (-0.002, 0.002)	0.52	1.00	1.00	1.00
Cadence [steps/minute]	112.6 (4.1)	112.6 (5.0)	0.05 (-0.63, 0.73)	0.44	1.00	1.00	1.00
Step Time [s]	0.54 (0.02)	0.54 (0.02)	0.00 (-0.002, 0.003)	0.28	1.00	1.00	1.00
Stance Time [s]	0.70 (0.02)	0.70 (0.03)	-0.005 (-0.02, 0.01)	0.001	0.98	0.98	0.98
Swing Time [s]	0.37 (0.02)	0.37 (0.02)	0.006 (-0.01, 0.02)	0.001	0.88	0.88	0.84
Double-Limb Support Time [s]	0.33 (0.04)	0.32 (0.04)	-0.01 (-0.05, 0.02)	0.003	0.87	0.87	0.84
Step Length [cm]	75.0 (3.1)	75.1 (3.6)	0.033 (-0.38, 0.45)	0.40	1.00	1.00	1.00
Stride Length [cm]	150.1 (3.6)	150.1 (3.8)	0.02 (-0.75, 0.79)	0.77	1.00	1.00	1.00
Stride Width [cm]	14.1 (1.4)	14.1 (1.5)	0.2 (-1.2, 1.2)	0.86	0.96	0.96	0.96



#### 4. Discussion

Spatiotemporal parameters are simple measures that effectively characterize gait patterns, allowing overall health status to be monitored and clinically meaningful changes to be detected. For this reason, researchers and clinicians have sought to incorporate them into clinical practice. The goal of this work was to determine if spatiotemporal gait parameters for healthy gait measured using a markerless motion capture system were equivalent to those from a marker-based motion capture system. If demonstrated with healthy gait and subsequently with impaired gait, this system could increase the clinical use and impact of spatiotemporal gait measurements. The findings presented here showed that spatiotemporal gait parameters from both systems demonstrated excellent agreement for healthy gait.

Marker-based motion capture is a widely accepted technology that can accurately measure spatiotemporal gait parameters; however, these systems are expensive, require dedicated laboratory space and experienced operators, and are time intensive to use. Currently, there are a wide variety of alternative technologies more suitable for clinical applications that have demonstrated the ability to accurately and reliably measure spatiotemporal gait parameters. Of the alternative technologies, pressure-sensitive walkways have had perhaps the greatest success in translation to clinical use due to their simplicity and ease of use. They have been implemented to study the gait patterns of children [24], older adults [25], individuals with Parkinson's disease [26], dementia [27], multiple sclerosis [28], and post-stroke patients [29] as a few examples. Despite the many benefits of these systems, they are limited to being used in straight, over-ground walking scenarios with their smooth, padded surface as the walking surface. These characteristics of the data collection process differ significantly from real-world walking, the majority of which is performed on inconsistent, rough surfaces with obstacles and turns to negotiate. Depth sensor-based technologies such as the Microsoft Kinect present another solution to collecting spatiotemporal gait data in clinical settings, and their validity has been demonstrated for several scenarios including over-ground walking [30], treadmill walking [31], and stair ambulation [32]. However, depth sensors have a limited range and it can be challenging to use more than one sensor without causing interference in their measurements, reducing the environments in which they can be used.

Markerless motion capture technology represents a simple and inexpensive technology that has a high potential for gait analysis given its lack of requirements of the walking surface, environment, or path. Previous work has been done towards using markerless motion capture technology for gait analysis, but this work is the first to validate spatiotemporal gait parameter measurements from a video-based markerless motion capture system against those from an accepted marker-based system for treadmill walking. The *Theia3D* markerless motion capture system does not require a specialized camera system, and is not limited by the collection environment. Without such restrictions, this system presents the opportunity to collect accurate spatiotemporal gait data at a reduced cost and time requirement compared to marker-based systems, and with the possibility of fully automating the analysis and reporting processes. We found that the two methods were indistinguishable for a variety of spatiotemporal gait parameters between the *Theia3D* markerless motion capture software and the marker-based motion capture system. The parameters with the lowest agreement and correlation were time-based measures whose differences were on scales similar to the duration of one camera frame ( $\sim 0.0118$  seconds). Considering the use of imperfect kinematic-based gait event detection methods that allowed independent events to be used for the two systems, the scale of the differences and the parameters in which they were observed are unsurprising. Any timing differences in the detection of gait events would affect the measurement of spatiotemporal gait parameters and increase the differences in measurements between the two systems, particularly for time-based parameters. Thus, it is reasonable to assume that the differences

between the markerless and marker-based spatial gait parameters would decrease when paired with force-detected gait events, however this work has demonstrated their similarity even without force-based event detection.

Despite the high level of agreement between spatiotemporal gait parameters measured using the marker-based and markerless motion capture systems, there are limitations to the present findings. The sample was comprised of healthy, active, young individuals which is not representative of the typically older, injured, or pathological population for which gait analysis is often used. In addition, the data collection was performed with participants walking on a treadmill. Since the markerless motion capture system is a purely image-based approach that examines each frame individually, its measurement of walking patterns is theoretically independent of the subject's health status and appearance, the collection environment, and whether they are walking over-ground or on a treadmill. However, the lack of sensitivity of the markerless system to these changes has yet to be confirmed. Subsequent work will investigate these factors and test the ability of markerless motion capture to measure spatiotemporal gait parameters in wider applications.

Based on the results presented here, the *Theia3D* markerless motion capture system is capable of accurately measuring spatiotemporal gait parameters of healthy adults during treadmill walking. In addition, markerless motion capture presents the potential to quickly collect large amounts of spatiotemporal gait data, reduce inter-operator and inter-laboratory effects present in marker-based motion capture, and allow data collection in realistic settings and conditions.

#### **Conflict of Interest Statement**

Scott Selbie is the President and Marcus Brown is the Director of Technology of Theia Markerless Inc. (Kingston, Ontario), the developers of *Theia3D*.

#### **Acknowledgements**

This work was supported by NSERC and the ISBS Developing Researcher Mobility Grant. We thank the members of the Human Mobility Research Laboratory for their assistance with participant recruitment, data collection, and data processing.

## References

- [1] B. Bilney, M. Morris, K. Webster, Concurrent related validity of the GAITRite® walkway system for quantification of the spatial and temporal parameters of gait, *Gait Posture*. 17 (2003) 68–74. [https://doi.org/10.1016/S0966-6362\(02\)00053-X](https://doi.org/10.1016/S0966-6362(02)00053-X).
- [2] E. Dolatabadi, B. Taati, A. Mihailidis, Concurrent validity of the Microsoft Kinect for Windows v2 for measuring spatiotemporal gait parameters, *Med. Eng. Phys.* 38 (2016) 952–958. <https://doi.org/10.1016/j.medengphy.2016.06.015>.
- [3] A. Gomez Bernal., R. Becerro-de-Bengoa-Vallejo, M.E. Losa-Iglesias, Reliability of the OptoGait portable photoelectric cell system for the quantification of spatial-temporal parameters of gait in young adults, *Gait Posture*. 50 (2016) 196–200. <https://doi.org/10.1016/j.gaitpost.2016.08.035>.
- [4] D. Trojaniello, A. Cereatti, E. Pelosin, L. Avanzino, A. Mirelman, J.M. Hausdorff, U. Della Croce, Estimation of step-by-step spatio-temporal parameters of normal and impaired gait using shank-mounted magneto-inertial sensors: application to elderly, hemiparetic, parkinsonian and choreic gait, *J. NeuroEngineering Rehabil.* 11 (2014) 152. <https://doi.org/10.1186/1743-0003-11-152>.
- [5] B.J. Braun, N.T. Veith, R. Hell, S. Döbele, M. Roland, M. Rollmann, J. Holstein, T. Pohlemann, Validation and reliability testing of a new, fully integrated gait analysis insole, *J. Foot Ankle Res.* 8 (2015) 54. <https://doi.org/10.1186/s13047-015-0111-8>.
- [6] A. Mathis, P. Mamidanna, K.M. Cury, T. Abe, V.N. Murthy, M.W. Mathis, M. Bethge, DeepLabCut: markerless pose estimation of user-defined body parts with deep learning, *Nat. Neurosci.* 21 (2018) 1281. <https://doi.org/10.1038/s41593-018-0209-y>.
- [7] M.W. Mathis, A. Mathis, Deep learning tools for the measurement of animal behavior in neuroscience, *Curr. Opin. Neurobiol.* 60 (2020) 1–11. <https://doi.org/10.1016/j.conb.2019.10.008>.
- [8] A. Mathis, P. Mamidanna, T. Abe, K.M. Cury, V.N. Murthy, M.W. Mathis, M. Bethge, Markerless tracking of user-defined features with deep learning, *ArXiv180403142 Cs Q-Bio Stat.* (2018). <http://arxiv.org/abs/1804.03142> (accessed January 13, 2020).
- [9] A. Elbaz, A. Mor, G. Segal, R. Debi, N. Shazar, A. Herman, Novel classification of knee osteoarthritis severity based on spatiotemporal gait analysis, *Osteoarthritis Cartilage*. 22 (2014) 457–463. <https://doi.org/10.1016/j.joca.2013.12.015>.
- [10] U. Givon, G. Zeilig, A. Achiron, Gait analysis in multiple sclerosis: Characterization of temporal–spatial parameters using GAITRite functional ambulation system, *Gait Posture*. 29 (2009) 138–142. <https://doi.org/10.1016/j.gaitpost.2008.07.011>.
- [11] M.R. Lemke, T. Wendorff, B. Mieth, K. Buhl, M. Linnemann, Spatiotemporal gait patterns during over ground locomotion in major depression compared with healthy controls, *J. Psychiatr. Res.* 34 (2000) 277–283. [https://doi.org/10.1016/S0022-3956\(00\)00017-0](https://doi.org/10.1016/S0022-3956(00)00017-0).
- [12] M.E. Morris, F. Huxham, J. McGinley, K. Dodd, R. Iansel, The biomechanics and motor control of gait in Parkinson disease, *Clin. Biomech.* 16 (2001) 459–470. [https://doi.org/10.1016/S0268-0033\(01\)00035-3](https://doi.org/10.1016/S0268-0033(01)00035-3).
- [13] J.H. Hollman, E.M. McDade, R.C. Petersen, Normative spatiotemporal gait parameters in older adults, *Gait Posture*. 34 (2011) 111–118. <https://doi.org/10.1016/j.gaitpost.2011.03.024>.
- [14] J. Fung, C.L. Richards, F. Malouin, B.J. McFadyen, A. Lamontagne, A Treadmill and Motion Coupled Virtual Reality System for Gait Training Post-Stroke, *Cyberpsychol. Behav.* 9 (2006) 157–162. <https://doi.org/10.1089/cpb.2006.9.157>.

- [15] S.L. Patterson, M.M. Rodgers, R.F. Macko, L.W. Forrester, Effect of treadmill exercise training on spatial and temporal gait parameters in subjects with chronic stroke: A preliminary report, *J. Rehabil. Res. Dev.* 45 (2008) 221–228.
- [16] E.M. Abd El-Kafy, H.M.Y.M. El-Basatiny, Effect of Postural Balance Training on Gait Parameters in Children with Cerebral Palsy, *Am. J. Phys. Med. Rehabil.* 93 (2014) 938. <https://doi.org/10.1097/PHM.000000000000109>.
- [17] N. Smania, P. Bonetti, M. Gandolfi, A. Cosentino, A. Waldner, S. Hesse, C. Werner, G. Bisoffi, C. Geroin, D. Munari, Improved Gait After Repetitive Locomotor Training in Children with Cerebral Palsy, *Am. J. Phys. Med. Rehabil.* 90 (2011) 137. <https://doi.org/10.1097/PHM.0b013e318201741e>.
- [18] C. Vitale, V. Agosti, D. Avella, G. Santangelo, M. Amboni, R. Rucco, P. Barone, F. Corato, G. Sorrentino, Effect of Global Postural Rehabilitation program on spatiotemporal gait parameters of parkinsonian patients: a three-dimensional motion analysis study, *Neurol. Sci.* 33 (2012) 1337–1343. <https://doi.org/10.1007/s10072-012-1202-y>.
- [19] B. Toro, C. Nester, P. Farren, A review of observational gait assessment in clinical practice, *Physiother. Theory Pract.* 19 (2003) 137–149. <https://doi.org/10.1080/09593980307964>.
- [20] T.-Y. Lin, M. Maire, S. Belongie, L. Bourdev, R. Girshick, J. Hays, P. Perona, D. Ramanan, C.L. Zitnick, P. Dollár, Microsoft COCO: Common Objects in Context, *ArXiv14050312 Cs.* (2015). <http://arxiv.org/abs/1405.0312> (accessed January 15, 2020).
- [21] J.A.Zeni Jr., J.G.Richards, J.S.Higginson, Two simple methods for determining gait events during treadmill and overground walking using kinematic data - ScienceDirect, *Gait Posture.* 27 (2008) 710–714. <https://doi.org/10.1016/j.gaitpost.2007.07.007>.
- [22] J. Martin Bland, Douglas G. Altman, STATISTICAL METHODS FOR ASSESSING AGREEMENT BETWEEN TWO METHODS OF CLINICAL MEASUREMENT, *The Lancet.* 327 (1986) 307–310. [https://doi.org/10.1016/S0140-6736\(86\)90837-8](https://doi.org/10.1016/S0140-6736(86)90837-8).
- [23] K.O. McGraw, S.P. Wong, Forming inferences about some intraclass correlation coefficients., *Psychol. Methods.* 1 (1996) 30–46. <https://doi.org/10.1037/1082-989X.1.1.30>.
- [24] L.M. Alderson, S.X. Joksaite, J. Kemp, E. Main, T. Watson, F.M. Platt, M. Cortina-Borja, Age-related gait standards for healthy children and young people: the GOS-ICH paediatric gait centiles, *Arch. Dis. Child.* 104 (2019) 755–760. <https://doi.org/10.1136/archdischild-2018-316311>.
- [25] S. Vallabhajosula, S.K. Humphrey, A.J. Cook, J.E. Freund, Concurrent Validity of the Zenon Walkway for Measuring Spatiotemporal Gait Parameters in Older Adults, *J. Geriatr. Phys. Ther.* 42 (2019) E42. <https://doi.org/10.1519/JPT.000000000000168>.
- [26] B. Mondal, S. Choudhury, R. Banerjee, K. Chatterjee, S. Ghosal, S.S. Anand, H. Kumar, Analysis of gait in Parkinson's disease reflecting the effect of l-DOPA, *Ann. Mov. Disord.* 2 (2019) 21. [https://doi.org/10.4103/AOMD.AOMD\\_19\\_18](https://doi.org/10.4103/AOMD.AOMD_19_18).
- [27] S.K.L. Darweesh, S. Licher, F.J. Wolters, P.J. Koudstaal, M.K. Ikram, M.A. Ikram, Quantitative gait, cognitive decline, and incident dementia: The Rotterdam Study, *Alzheimers Dement.* 15 (2019) 1264–1273. <https://doi.org/10.1016/j.jalz.2019.03.013>.
- [28] K. Novotna, J. Rusz, E. Kubala Havrdova, J. Lizrova Preiningerova, Why patients with multiple sclerosis perceive improvement of gait during treatment with natalizumab?, *J. Neural Transm.* 126 (2019) 731–737. <https://doi.org/10.1007/s00702-019-02013-z>.
- [29] B.T. Cleland, H. Arshad, S. Madhavan, Concurrent validity of the GAITRite electronic walkway and the 10-m walk test for measurement of walking speed after stroke, *Gait Posture.* 68 (2019) 458–460. <https://doi.org/10.1016/j.gaitpost.2018.12.035>.

- [30] B. Müller, W. Ilg, M.A. Giese, N. Ludolph, Validation of enhanced kinect sensor based motion capturing for gait assessment, *PLOS ONE*. 12 (2017) e0175813. <https://doi.org/10.1371/journal.pone.0175813>.
- [31] M. Eltoukhy, J. Oh, C. Kuenze, J. Signorile, Improved kinect-based spatiotemporal and kinematic treadmill gait assessment, *Gait Posture*. 51 (2017) 77–83. <https://doi.org/10.1016/j.gaitpost.2016.10.001>.
- [32] J. Oh, C. Kuenze, M. Jacopetti, J.F. Signorile, M. Eltoukhy, Validity of the Microsoft Kinect™ in assessing spatiotemporal and lower extremity kinematics during stair ascent and descent in healthy young individuals, *Med. Eng. Phys.* 60 (2018) 70–76. <https://doi.org/10.1016/j.medengphy.2018.07.011>.
- [33] M. Almarwani, S. Perera, J.M. VanSwearingen, P.J. Sparto, J.S. Brach, The test–retest reliability and minimal detectable change of spatial and temporal gait variability during usual over-ground walking for younger and older adults, *Gait Posture*. 44 (2016) 94–99. <https://doi.org/10.1016/j.gaitpost.2015.11.014>.
- [34] J.E. Wittwer, K.E. Webster, K. Hill, Reproducibility of gait variability measures in people with Alzheimer’s disease, *Gait Posture*. 38 (2013) 507–510. <https://doi.org/10.1016/j.gaitpost.2013.01.021>.
- [35] R.W. Bohannon, S.S. Glenney, Minimal clinically important difference for change in comfortable gait speed of adults with pathology: a systematic review, *J. Eval. Clin. Pract.* 20 (2014) 295–300. <https://doi.org/10.1111/jep.12158>.
- [36] P.M. Nair, G. Hornby T., A.L. Behrman, Minimal Detectable Change for Spatial and Temporal Measurements of Gait After Incomplete Spinal Cord Injury, *Top. Spinal Cord Inj. Rehabil.* 18 (2012) 273–281. <https://doi.org/10.1310/sci1803-273>.